


Title : IMG1

Instrument : 6390 (LA)
 Volt : 30.00 kV
 Mag. : x 40
 Date : 2010/03/31
 Pixel : 512 x 384

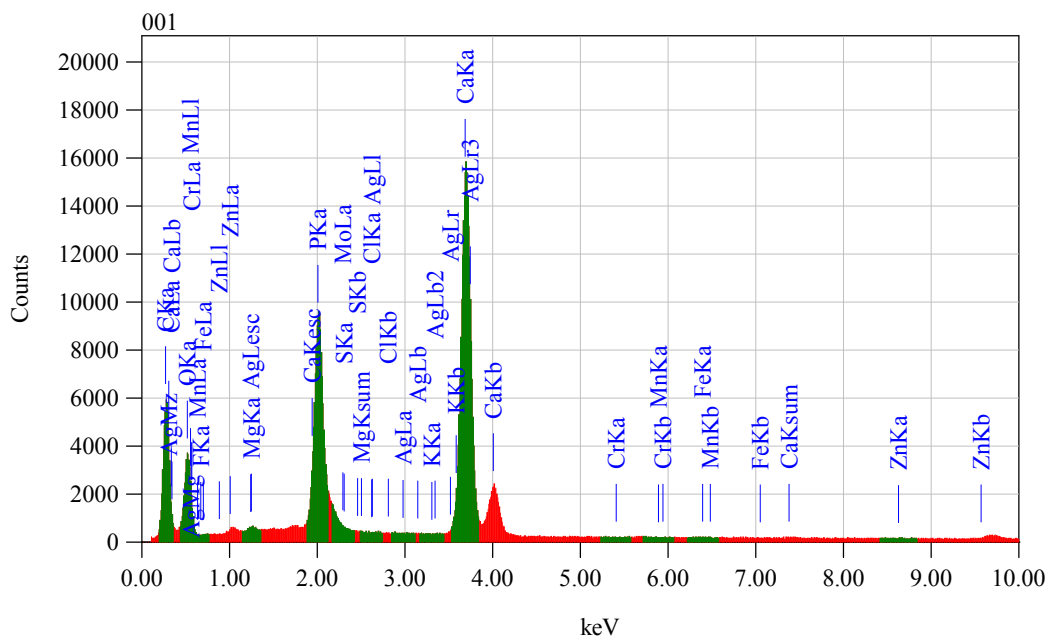

Acquisition Parameter
 Instrument : 6390 (LA)
 Acc. Voltage : 30.0 kV
 Probe Current: 1.00000 nA
 PHA mode : T2
 Real Time : 59.28 sec
 Live Time : 45.00 sec
 Dead Time : 22 %
 Counting Rate: 19945 cps
 Energy Range : 0 - 20 keV

ZAF Method Standardless Quantitative Analysis

Fitting Coefficient : 0.2975

Element	(keV)	Mass%	Error%	Atom%	Compound	Mass%	Cation	K
C	0.277	45.68	0.17	57.14				20.0584
O	0.525	38.78	0.76	36.42				21.5246
F								
Mg	1.253	0.17	0.10	0.10				0.1074
P	2.013	5.22	0.07	2.53				10.6881
S								
Cl	2.621	0.01	0.05	0.01				0.0226
K	3.312	0.12	0.06	0.04				0.2096
Ca	3.690	9.97	0.07	3.74				18.1509
Cr	5.411	0.01	0.12	0.00				0.0103
Mn	5.894	0.00	0.13	0.00				0.0003
Fe	6.398	0.04	0.13	0.01				0.0574
Zn								
Mo								
Ag								
Total		100.00		100.00				