



ХИМИЧЕСКИЙ СОСТАВ МИНЕРАЛИЗОВАННОГО КОРТИКАЛЬНОГО ПОРОШКА "ЛИОПЛАСТ-С" ®

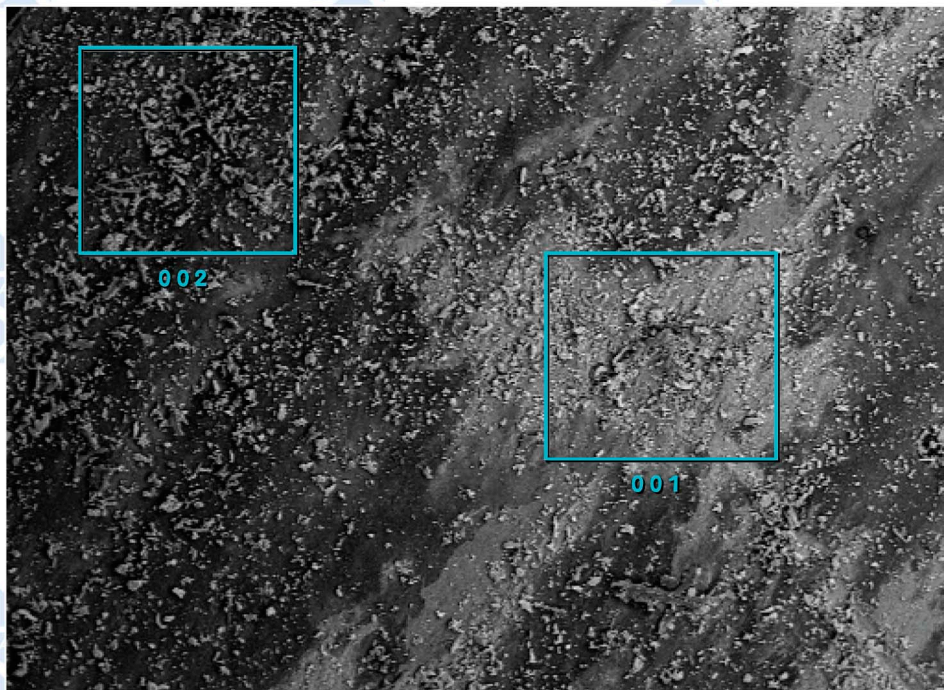

Title : IMG1
 Instrument : 6390 (LA)
 Volt : 30.00 kV
 Mag. : x 40
 Date : 2010/03/31
 Pixel : 512 x 384

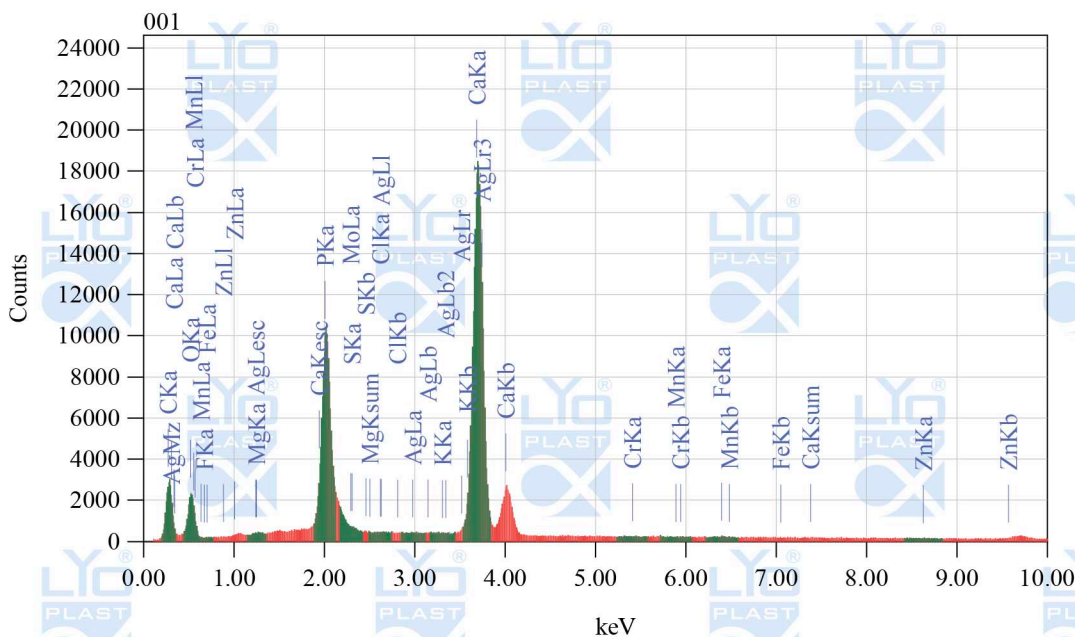

Acquisition Parameter
 Instrument : 6390 (LA)
 Acc. Voltage : 30.0 kV
 Probe Current : 1.00000 nA
 PHA mode : T2
 Real Time : 58.26 sec
 Live Time : 45.00 sec
 Dead Time : 22 %
 Counting Rate : 18160 cps
 Energy Range : 0 - 20 keV

ZAF Method Standardless Quantitative Analysis
 Fitting Coefficient : 0.2288


Element	(keV)	Mass%	Error%	Atom%	Compound	Mass%	Cation	K
C	0.277	38.26	0.22	51.57				11.1680
O	0.525	36.75	1.04	37.18				15.4473
F	0.677	0.46	0.84	0.39				0.0414
Mg	1.253	0.12	0.11	0.08				0.0648
P	2.013	7.76	0.07	4.06				13.2028
S								
Cl	2.621	0.03	0.06	0.02				0.0472
K	3.312	0.15	0.06	0.06				0.2320
Ca	3.690	16.34	0.07	6.60				24.5861
Cr	5.411	0.02	0.12	0.01				0.0237
Mn								
Fe	6.398	0.08	0.14	0.02				0.0920
Zn	8.630	0.01	0.28	0.00				0.0155
Mo								
Ag								
Total		100.00		100.00				

КОНТАКТЫ

lyoplast.ru
 lyoplast.com


russianboneblocks.ru

ХИМИЧЕСКИЙ СОСТАВ МИНЕРАЛИЗОВАННОГО СПОНГИОЗНОГО ПОРОШКА "ЛИОПЛАСТ-С" ®

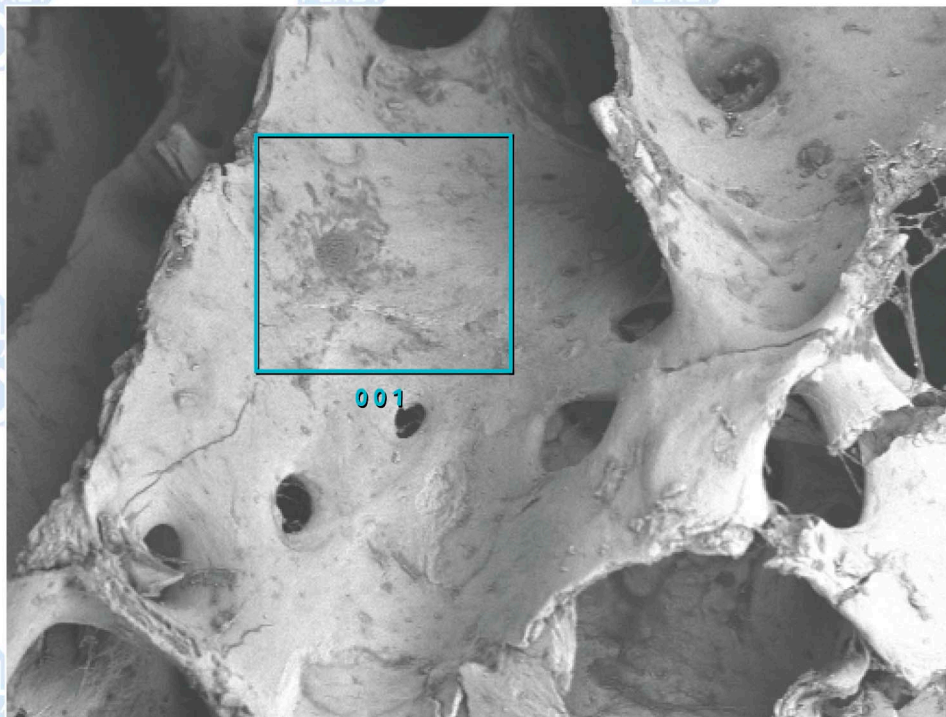

1.0 mm

Title : IMG1
 Instrument : 6390 (LA)
 Volt : 30.00 kV
 Mag. : x 40
 Date : 2010/03/31
 Pixel : 512 x 384

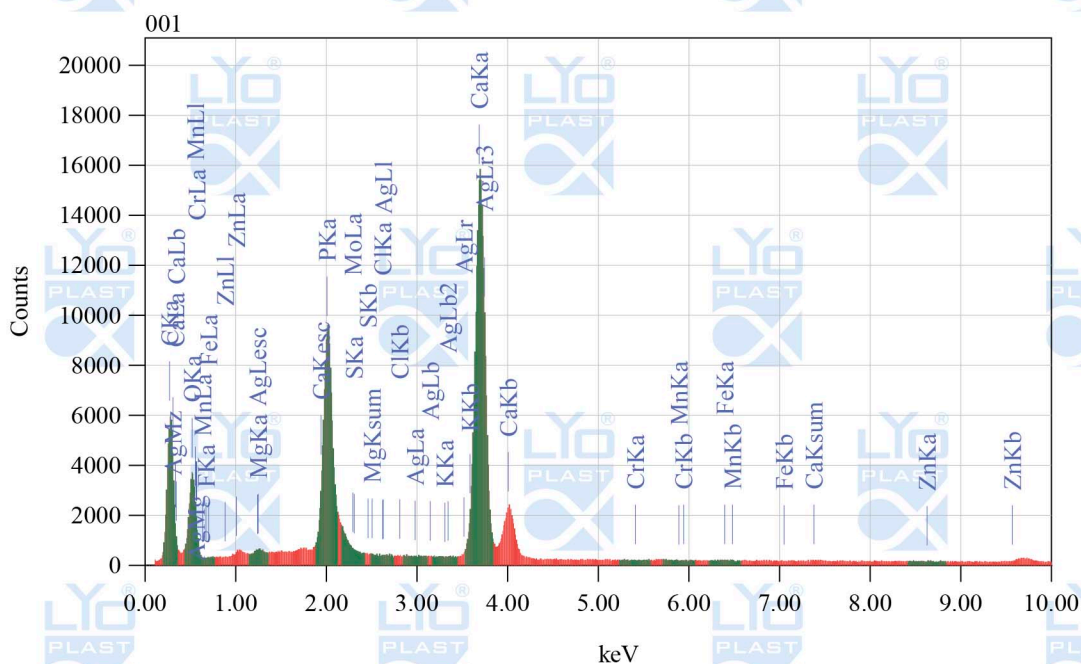


Acquisition Parameter
 Instrument : 6390 (LA)
 Acc. Voltage : 30.0 kV
 Probe Current : 1.00000 nA
 PHA mode : T2
 Real Time : 59.28 sec
 Live Time : 45.00 sec
 Dead Time : 22 %
 Counting Rate : 19945 cps
 Energy Range : 0 - 20 keV


ZAF Method Standardless Quantitative Analysis
 Fitting Coefficient : 0.2975

Element	(keV)	Mass%	Error%	Atom%	Compound	Mass%	Cation	K
C	0.277	45.68	0.17	57.14				20.0584
O	0.525	38.78	0.76	36.42				21.5246
F								
Mg	1.253	0.17	0.10	0.10				0.1074
P	2.013	5.22	0.07	2.53				10.6881
S								
Cl	2.621	0.01	0.05	0.01				0.0226
K	3.312	0.12	0.06	0.04				0.2096
Ca	3.690	9.97	0.07	3.74				18.1509
Cr	5.411	0.01	0.12	0.00				0.0103
Mn	5.894	0.00	0.13	0.00				0.0003
Fe	6.398	0.04	0.13	0.01				0.0574
Zn								
Mo								
Ag								
Total		100.00		100.00				

ХИМИЧЕСКИЙ СОСТАВ ДЕМИНЕРАЛИЗОВАННОГО КОРТИКАЛЬНОГО ПОРОШКА "ЛИОПЛАСТ-С" ®

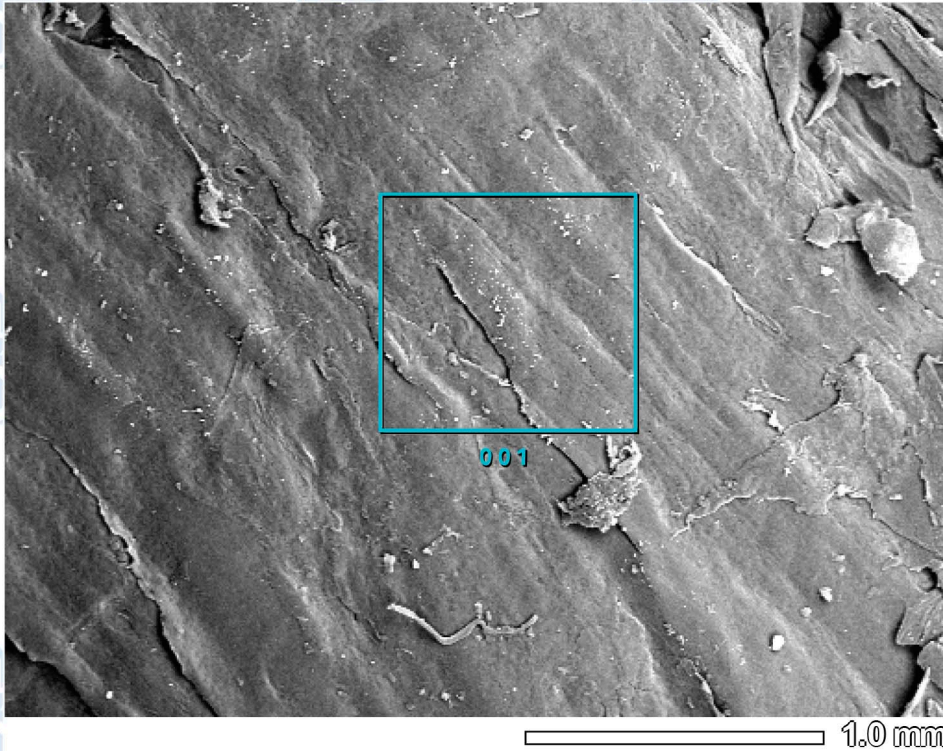

Title	: IMG1
Instrument	: 6390 (LA)
Volt	: 30.00 kV
Mag.	: x 40
Date	: 2010/03/31
Pixel	: 512 x 384

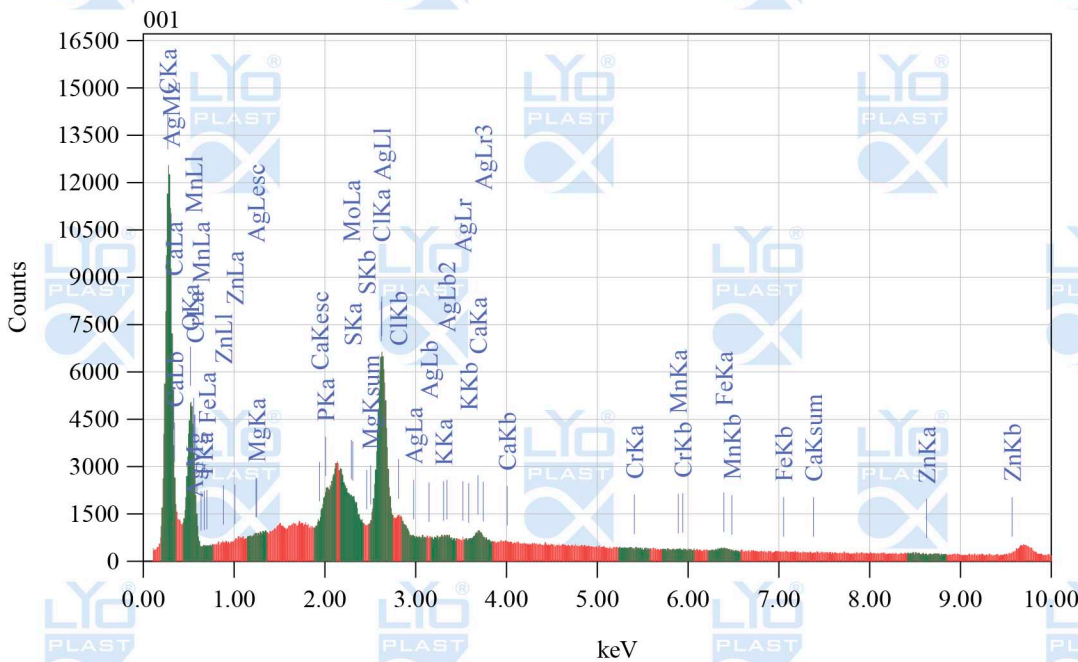


Acquisition Parameter	
Instrument	: 6390 (LA)
Acc. Voltage	: 30.0 kV
Probe Current	: 1.00000 nA
PHA mode	: T2
Real Time	: 60.43 sec
Live Time	: 45.00 sec
Dead Time	: 25 %
Counting Rate	: 21212 cps
Energy Range	: 0 - 20 keV

ZAF Method Standardless Quantitative Analysis
Fitting Coefficient : 0.3559

Element	(keV)	Mass%	Error%	Atom%	Compound	Mass%	Cation	K
C	0.277	60.23	0.08	67.72				46.0117
O	0.525	37.02	0.39	31.25				31.1130
F								
Mg								
P								
S	2.307	0.12	0.03	0.05				0.3283
Cl	2.621	2.31	0.03	0.88				5.7557
K	3.312	0.05	0.04	0.02				0.1281
Ca	3.690	0.16	0.04	0.05				0.3921
Cr								
Mn	5.894	0.01	0.07	0.00				0.0229
Fe	6.398	0.10	0.07	0.02				0.1894
Zn								
Mo								
Ag								
Total		100.00		100.00				


ХИМИЧЕСКИЙ СОСТАВ ДЕМИНЕРАЛИЗОВАННОГО СПОНГИОЗНОГО ПОРОШКА "ЛИОПЛАСТ-С" ®

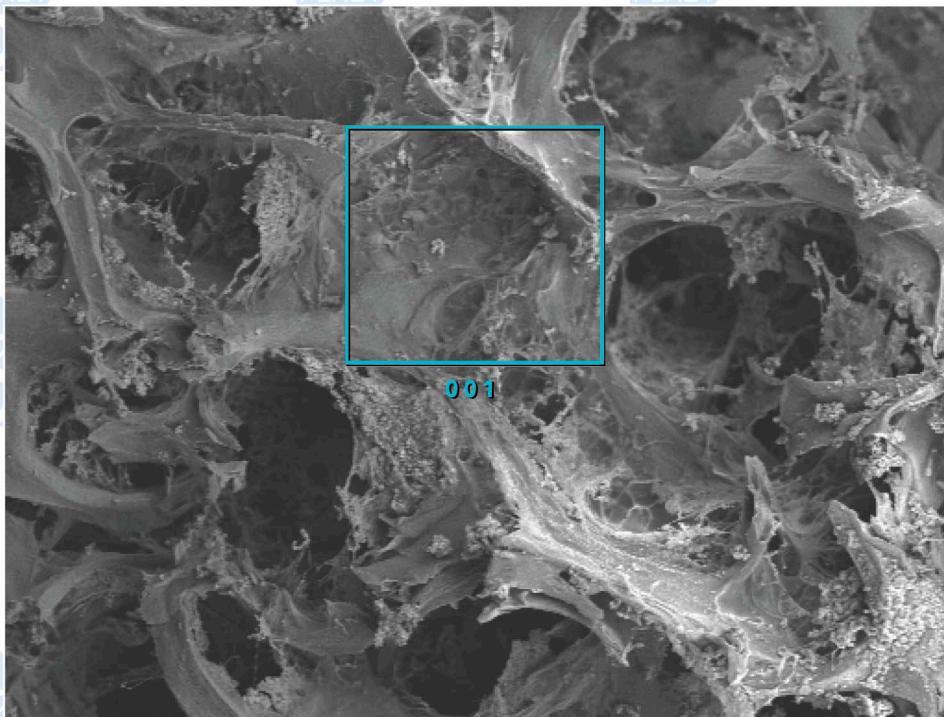

Title : IMG1
 Instrument : 6390 (LA)
 Volt : 30.00 kV
 Mag. : x 40
 Date : 2010/03/31
 Pixel : 512 x 384

001

1.0 mm

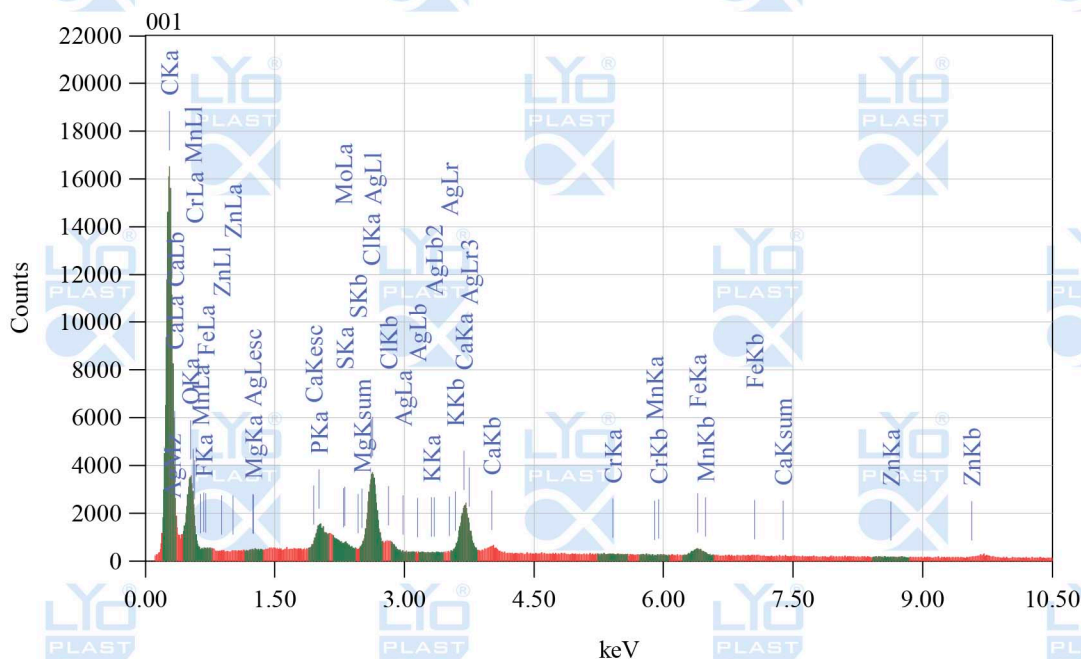

Acquisition Parameter
 Instrument : 6390 (LA)
 Acc. Voltage : 30.0 kV
 Probe Current : 1.00000 nA
 PHA mode : T2
 Real Time : 56.94 sec
 Live Time : 45.00 sec
 Dead Time : 20 %
 Counting Rate : 18289 cps
 Energy Range : 0 - 20 keV

ZAF Method Standardless Quantitative Analysis
 Fitting Coefficient : 0.4057

Element	(keV)	Mass%	Error%	Atom%	Compound	Mass%	Cation	K
C	0.277	67.49	0.13	74.58				56.5541
O	0.525	29.26	0.98	24.27				18.1092
F								
Mg	1.253	0.04	0.11	0.02				0.0298
P	2.013	0.34	0.07	0.14				0.8794
S	2.307	0.03	0.05	0.01				0.0746
Cl	2.621	1.38	0.06	0.52				3.1548
K	3.312	0.02	0.07	0.01				0.0357
Ca	3.690	1.09	0.08	0.36				2.4692
Cr	5.411	0.01	0.13	0.00				0.0108
Mn								
Fe	6.398	0.36	0.15	0.08				0.6270
Zn								
Mo								
Ag								
Total		100.00		100.00				